ENGINEERING NOTE

LH2003 Draft(r2) Page 1 of 13

Page

Serial #

Author Department Date

Jon Zbasnik Mechanical Engineering 21 Oct 2002

Cat. Code

<u>Program - Project - Job</u>: <u>LHC IR Feedboxes</u> Cryogenics

Title: Lambda Plug R&D Report

1. Introduction

The DFBX requires two types of bus bar plugs that separate the 4.5K liquid helium vessel of the DFBX from the pressurized superfluid helium volume of the superconducting inner triplet quadrupoles and separation dipoles. The plugs are called lambda plugs, after the term "lambda transition" that is used to represent the superfluid to normal transition because the specific heat variation with temperature around the transition temperature has the shape of the greek letter "lambda".

One type connects to Q3, the outermost quadrupole magnet of the LQX assembly. This bus consists of 4 high-current conductors and 24 lower current conductors. The high current conductors each carry up to 7500 A and the lower current conductors each carry up to 600 A. Eight of these are required, one for each DFBX. This type is designated as the Q3 Lambda Plug

The other type connects to the superconducting D1 that is deployed at points 2 and 8 of the LHC. This bus requires 2 high current conductors to power the "A" and "B" leads of the superconducting D1. The conductors must carry up to 6000 A. Four of these are required, one for each of the DFBX at points 2 and 8. This type is designated as the D1 Lambda Plug.

This report presents the requirements, design features, fabrication outline, and test results of the LBNL R&D lambda plug for the DFBX.

2. Requirements

2.1 Electrical Requirements

- 2.1.1 Current Rating for Q3 Type
 - 4 busses each with a 7500 A capability to power main inner triplet quadrupoles
 - 24 busses each with a 600 A capability to power inner triplet corrector magnets
- 2.1.2 Current Rating for D1 Type
 - 2 busses each with 7500 A capability to power D1 separation dipole
- 2.1.3 Voltage Rating for Q3 and D1 Types

For each 7500 A conductor, 1500 VDC in STP helium or 5000 VDC in STP air, with all other conductors at ground potential.

Leakage current to be less than 20 x 10⁻⁶ A after 1 minute at voltage. For each 600 A conductor, 600 VDC in STP helium or 2500 VDC in STP air, with all other conductors at ground potential.

ENGINEERING NOTE

LH2003 Draft(r2) Page 2 of 13

Page

Serial #

Author Department Date

Jon Zbasnik Mechanical Engineering 21 Oct 2002

Cat. Code

Leakage current to be less than 20 x 10⁻⁶ A after 1 minute at voltage.

2.2 Mechanical Requirements

- 2.2.1 Magnet-Side Pressure Rating for Q3 and D1 types
 - 20 bar abs. (275 psig) Design Pressure
 - 30 bar abs. (420 psig) Test Pressure for R&D Plugs
 - 25 bar gauge (365 psig) Test Pressure for Production Plugs
- 2.2.1 DFBX-side Pressure Rating for Q3 and D1 type
 - 3.5 bar abs. (51 psig) Design Pressure
 - 5.5 bar gauge (80 psig) Test Pressure for R&D Plugs
 - 4.5 bar gauge (65 psig) Test Pressure for Production Plugs
- 2.2.3 Leakage Rate for O3 and D1 types

Less than 0.1 atm - cc/s (helium) at Room Temperature (10 Pa-l/s)

- 2.3 Operational Requirements (These are to be satisfied in R&D program)
 - 2.3.1 Thermal Cycles for Q3 and D1 Types

Satisfy leak rate in 2.2.3 after 50 thermal cycles (300 K \Rightarrow 80K \Rightarrow 300K)

2.3.2 Magnet Ouenches for O3 and D1 Types

Satisfy leak rate in 2.2.2 after 25 pressure pulses of Design Pressure in 2.2.1

2.4 Other Constraints

Production Process must be stable and repeatable

Must allow for reliable attachment to the DFBX helium vessel

Bus bars must be stable against quenching:

use the 7500 A bus developed by FNAL for the inner triplet quadrupoles use the 600 A LHC rectangular corrector bus wire

3. Determination of Acceptable Leak Rate

We performed an experimental determination of the leak rate of air through a small diameter tube. The tube had a 0.006 inch (0.15 mm) diameter and was 2 inch (50 mm long). It is actually a 30 gauge stainless steel dispensing needle purchased from McMaster-Carr Supply Company that provided a convenient leak calibration standard.

Using a critical heat flux of 5.5 W/cm², the superfluid heat load for a 0.15 mm diameter path is approximately 1 mW. Compared with the heat load from conduction through the materials in the lambda plug, about 4 W for the worst case, this represents a negligible contribution.

Another consideration, from Tom Peterson, is that we want to limit the mass flow from the magnets into the DFBX helium chamber. The worst-case mass flow through a 0.15

ENGINEERING NOTE

Draft(r2) Page 3 of 13 LH2003 Author Department Date Jon Zbasnik **Mechanical Engineering** 21 Oct 2002

Cat. Code

Serial #

Page

mm diameter path through the lambda plug will be about 0.035 g/s for a 1.7 bar pressure differential. This rate is less than the specified leakage rate across the CERN superfluid safety relief valves of .01 g/sec for a 0.1 bar pressure differential and therefore is acceptable for LHC operation.

A final consideration is that the small diameter path will limit mass flow during high pressure tests at LBNL, the DFBX Vendor site, and at CERN to levels that will minimize the impact on carrying out the tests.

The leak rate through the needle was determined using a classical rate of rise measurement in which a closed volume was evacuated and then allowed to be pressurized by atmospheric pressure through the needle. Figure 3 –1 shows the test setup used

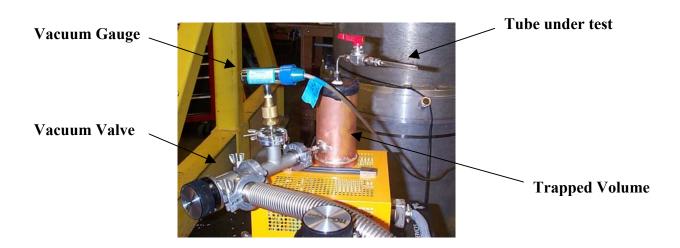


Figure 3-1. Rate of Rise Test Setup.

The pressure reading as a function of time is shown in Figure 3-2.

Author

LH2003 Draft(r2) Page 4 of 13 Department Date Jon Zbasnik **Mechanical Engineering** 21 Oct 2002

Cat. Code

Serial #

Page

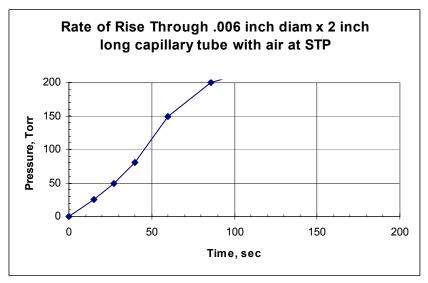


Figure 3-2. Rate of Rise Results.

The volume of the trapped volume is 310 cm³ (0.31 liter) and we see that the pressure rose 200 Torr in 86 sec. The leak rate is therefore,

Leak rate = 200 Torr x .31 liter/86 s = 0.72 Torr-l/s (air)
=
$$0.72 \times 1.33 = 0.96$$
 atm cc/s (air)
= $0.96 \times 2.7 = 2.6$ atm cc/s (helium)

Therefore, our requirement that the leak rate of the lambda plug shall be less than 0.1 atm cc/s (helium), as stated in 2.2.3 above, gives a very large safety margin in performance since the leak rate could be as high as 2.6 atm cc/sec (helium) and still be acceptable for LHC operation.

4. Lambda Plug Design and Fabrication

The basic concept of the design is to pot the conductors in an insulating block of NEMA G10-CR, and then pot this in a stainless steel housing.

Figure 4-1 shows an R&D version (PG-4) of the plug. The outer diameter of the stainless steel housing is 6 inch (152 mm) and it tapers as a conventional weldneck pipe flange to the 3.5 inch (88.9 mm) outer diameter pipe on the right hand side. In Figure 4-1 the conductors are about 8 inch (200 mm) long whereas in the production versions they will be about 96 inch (2.44 m) long.

Author Department Date

Jon Zbasnik Mechanical Engineering 21 Oct 2002

Cat. Code

LH2003

Serial #

Draft(r2)

Page

Page 5 of 13

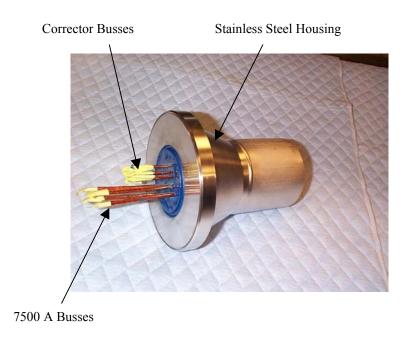


Figure 4-1. R&D lambda Plug Assembly

Figure 4-2 shows R&D Plug PG-4 with its closeout welding completed. The left side simulates how the lambda plug assembly will attached to the bus duct at LBNL, and the right side simulates the field welding that will performed by the Vendor to seal weld the bus duct assembly to the DFBX liquid helium vessel. The clamping ring provides mechanical support for the seal weld. A sketch of the cross section is shown in Figure 4-2.1.

Author Department Date

Jon Zbasnik Mechanical Engineering 21 Oct 2002

Cat. Code

LH2003

Serial #

Draft(r2)

Page

Page 6 of 13

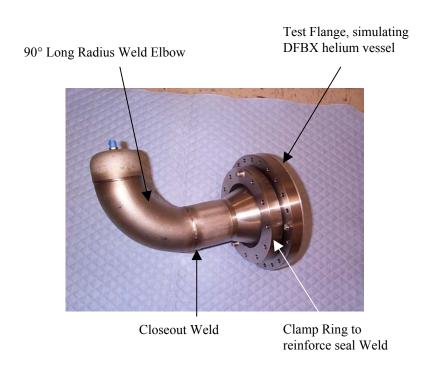


Figure 4-2. R&D Lambda Plug with closeout welding completed.

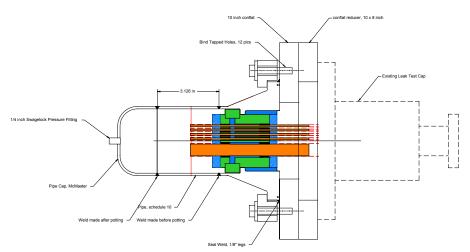


Figure 4.2-1 Cross-section of Lambda Plug

Author Department Date

Jon Zbasnik Mechanical Engineering 21 Oct 2002

Cat. Code

LH2003

Serial #

Draft(r2)

Page

Page 7 of 13

The heart of the lambda plug assembly is a two-piece NEMA G-10CR insulator block shown in Figure 4-3. The design allows for proper spacing and orientation of the conductors. The plane of reinforcement is parallel to the faces of the plug. After the two parts are assembled, the configuration allows for the conductors to be encapsulated in Stycast 2850MT (blue) epoxy, using hardener 24LV.

Figure 4-4 shows some of the steps in filling the Rutherford cables with 60/40 Sn/Pb solder. Solder foils are inserted into the cable, following a suggestion from V. Benda of CERN, to ensure that the interior of the cable is completely filled with solder. The cable with the inserted foils, along with additional solder foils, are laid into the heater box where the parts are heated with cartridge heaters. Heat sinks are used to prevent the solder from wicking beyond the area that will be potted in the insulator block.

Figure 4-5 shows the insulated busses, and the gap in their insulation that will be located inside the insulator block can be seen.






Figure 4-3. DFBX Lambda Plug Insulator Block

Author Department Date

Jon Zbasnik Mechanical Engineering 21 Oct 2002

Cat. Code

LH2003

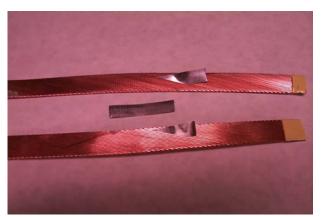

Solder-Filling the Cable



Serial #

Draft(r2)

Page


Page 8 of 13

Flowing the Solder with Heaters

Figure 4-4. Cable Filling Steps



7500 A Main Magnet Busses

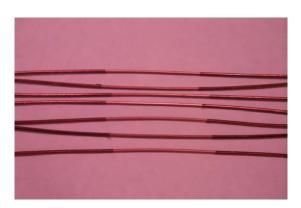

600 A Corrector Busses

Figure 4-5. Insulated Busses

Author Department

Jon Zbasnik Mechanical Engineering 21 Oct 2002

Cat. Code

LH2003

Serial #

Draft(r2)

Page

Date

Page 9 of 13

The insulated conductors are potted in the insulator block with Stycast 2850MT (blue) with 24LV hardener by a two-step process shown in Figure 4-6. The procedure is quite detailed and careful attention must be given to surface preparation, handling, and environmental control.

After 3 thermal cycles and a leak check to verify leak-tightness the insulator block is potted in the stainless housing using Stycast 2850MT (blue) with hardener 24LV.



Step 1 - Potting the "magnet" end



Step 2 – Fill the Insulator Block by Injection in Vacuum Chamber



Potting Chamber

Figure 4-6. Potting the Conductors in the Insulator Block

ENGINEERING NOTE

Author	Department	
Jon Zbasnik	Mechanical Engineering	21 Oct 2002

Cat. Code

LH2003

Serial #

Draft(r2)

Page

Page 11 of 13

The final step in the fabrication of the R&D Lambda Plugs is the closeout and seal welding. The welding simulates the anticipated thermal stresses that would be encountered in the actual fabrication and installation.

The weld to the 3.5 inch section is done by:

- installing a backing ring on the piping that will be welded to the lambda plug,
- tack welding the pieces into the proper position,
- making a GTAW fusion root pass with 1-inch (25 mm) long welds, skipping around the circumference to control distortion, pausing between skips to allow the part to be cooled to room temperature between skips with a "Cool Gun",
- making a GTAW seal pass with ER316L filler wire, skipping, pausing, and cooling as was done in the fusion root pass
- the temperature at the area of the epoxy potting is maintained below 30C

The weld to the test flange, simulating the welding required to attach the lambda Plug Assembly to the DFBX liquid helium vessel, is also done in a discontinuous manner using 1 inch (25 mm) long welds, pausing between welds and allowing the part to be cooled to room temperature with a "Cool Gun" between welds. Originally, we assumed the weld to be a fillet weld with 0.125 inch (3.2 mm) legs, but we found that we could reduce the fillet leg to 0.06 inch. Welding is done using the GTAW process; the 0.125 fillet required ER316L filler wire to be used, but the 0.06 fillet can be made with a fusion process. The temperature of the epoxy regions is maintained below 30C during this welding.

5. DFBX Lambda Plug R&D Testing Results

The final series of R&D lambda plugs is designated as PG-6, and consist of 5 samples,

PG-6a: Insulated main conductors, insulated corrector conductors, 0.125 fillet weld

PG-6b: Mixed too much epoxy; this hardened prematurely due to exotherm heating, prevented proper potting

PG-6c: Insulated main conductors, bare corrector conductors, 0.125 fillet weld

PG-6d: Insulated main conductors, bare corrector conductors, 0.06 fillet weld

PG-6e: No conductors (solid G-10 plug), 0.06 fillet weld.

A summary of the test results is given in Tables 5-1.

ENGINEERING NOTE

Daniel Date

Author Department Date

Jon Zbasnik Mechanical Engineering 21 Oct 2002

Table 5-1. Summary of R&D Tests on PG-6 series Lambda Plugs

Test Sequence	PG-6a	PG-6b	PG-6c	PG-6d	PG-6e ^f
In-Process Testing	All okay	Incomplete	All okay	All okay	
		step 2 potting ^a			
Leak rate after potting		Plug was		<1 x 10 ⁻¹⁰	
in housing		not used		atm cc/s	
Leak Rate after 2			<1 x 10 ⁻¹⁰	<1 x 10 ⁻¹⁰	
thermal cycles			atm cc/s	atm cc/s	
Leak Rate after welding	.035		.069	7 x 10 ⁻¹⁰	
_	atm cc/s b		atm cc/s c	atm cc/s	
50 thermal cycles ^d	done		done	done	
Post-thermal cycling	.035		0.10	3.6 x 10 ⁻³	
leakage	atm cc/s		atm cc/s	atm cc/s	
R.T. Pressure Test to	Passed,		Passed, not	Passed, not	
420 psig (29 bar)	not		deformed	deformed	
	deformed			2	
Post-pressure test	.035		0.1	7.5×10^{-3}	
leakage	atm cc/s		atm cc/s	atm cc/s	
Cold Pressure Test to	Passed,		Passed, not	Passed, not	
420 psig	not		deformed	deformed	
	deformed				
25 quench pressure	Not done		Passed	Passed	
pulses					
Post-pressure test	.025		.069	6.1 x 10 ⁻³	
leakage	atm cc/s		atm cc/s	atm cc/s	
R.T. Pressure test	Not done		Passed	Passed	
DFBX side to 80 psig					
Cold Pressure test	Not done		Passed	Passed	
DFBX side to 80 psig					
7500 A HiPot to 5 kV	Ok to 5				
	kV in air				
600 A HiPot to 2.5 kV	22 ok to				
	2.5 kV in				
	air ^e				

Notes:

- a. An excessive amount (1000 g) of epoxy was mixed and the exothermic heat generated caused the epoxy to harden before the plug was filled.
- b. No change in leak rate due to welding.
- c. We have evidence that the leak rate increased upon welding. We will check this carefully in PG-6d.
- d. Thermal cycling is done by plunging the assembly into a bath of LN_2 , held for 1 hr, then pulled out and warmed in air for 1 hour, etc.
- e. Breakdown is not between nearest neighbors, so it may be due to the test setup. We are checking this.
- f. In test as of 21 Oct 2002.

ENGINEERING NOTE

ENGINEERING NOTE	LH2003	Draft(r2)	Page 13 of 13
41	D		D-4-

Cat. Code

Serial #

Page

Author Department Date

Jon Zbasnik **Mechanical Engineering** 21 Oct 2002

6. Conclusions

- The R&D results on the PG-6 series plugs demonstrate that we have developed a lambda plug that meets the requirements stated in section 2.
- The room temperature leak rate requirement of 0.1 atm cc/sec (helium) provides an operational safety factor of about 10 when compared to the leak requirement for the CERN pressure safety relief valves on the pressurized superfluid system.
- We have made three plugs in a row with conductors that satisfy the leak rate requirement after thermal cycling and pressure testing at room temperature and liquid nitrogen temperature.
- The testing included simulation of the welding needed to carryout the closeout of the bus duct piping and also the welding needed to attach the lambda plug assembly to the DFBX liquid helium vessel.
- A fourth plug was made without conductors to provide additional confidence that the seal weld to the DFBX liquid helium vessel will not cause excessive degradation of the bond between the stainless steel housing and the G-10 insulator block.